



CR imaging plate system

Certificate N°: BAM/ZBF/003/16



Bundesanstalt für
Materialforschung
und -prüfung

Hereby it is certified by the BAM Certification Body that the

Industrial CR imaging plate system

with the designation

CR^xFlex type 5176/200

in combination with

GE Inspection Technologies phosphor imaging plates IPU

meets the requirements of the highest CR system class IP 1 / 50 according to EN 14784-1:2005 and ISO 16371-1:2011, if the exposure dose is at minimum 2.0 mGy, for industrial computed radiography with phosphor imaging plates. This dose corresponds to a CEN speed and ISO speed of 500 at a pixel size of 50 µm. CR system performance level II according to ASTM E 2446-15 for non-destructive testing is fulfilled at an ISO speed of 2000. The maximum basic spatial resolution is 50 µm. Other system classes (CEN/ISO: IP 2 / 50 to IP 6 / 50) and CR system performance levels (ASTM: level III) can be achieved with lower exposure dose values (see test report No. 8.3 / 7997b of 2016-04-29 for all characterization data). The spider net graph with the summary of the CR system characterization according to ASTM E2446-15 is presented on the back side of this certificate.

Certificate holder according to certification contract No. BAM-ZBA-0014-2006-GE IT:

GE Sensing & Inspection Technologies GmbH, Ahrensburg, Germany

System manufactured by AGFA HEALTHCARE N.V. in Germany.

The certification is performed according to standard ISO/IEC 17065:2012 and comprises a design type test (BAM Certification System I).

The products certified by BAM may be labeled with the BAM certification mark „BAM Baumustergeprüft“ and/or “BAM Design-type tested” together with the certificate number.

The certificate is valid until May 8th, 2020.

For Bundesanstalt für Materialforschung und -prüfung (BAM)
Unter den Eichen 87, 12205 Berlin, **2016-05-09**

Dr. R. Schmidt
BAM Certification Body



Dr. U. Ewert
BAM Assessor

Distribution list:: 1st Certificate holder

2nd BAM Certification Body


The BAM Certification Body has been accredited according to standard ISO/IEC 17065:2012 by the DAkkS (Deutsche Akkreditierungsstelle GmbH). The accreditation is valid for the scope given in certificate D-ZE-11075-21-00.

This certificate may only be published in full wording and without any additions. A revocable written consent shall be obtained from BAM beforehand for any amended reproduction or the publication of any excerpts. The German version is legally binding, except an English version is issued exclusively. Place of jurisdiction is Berlin.

Sicherheit in Technik und Chemie

CERTIFICATE

Qualification of CR^xFlex system with IPU plates

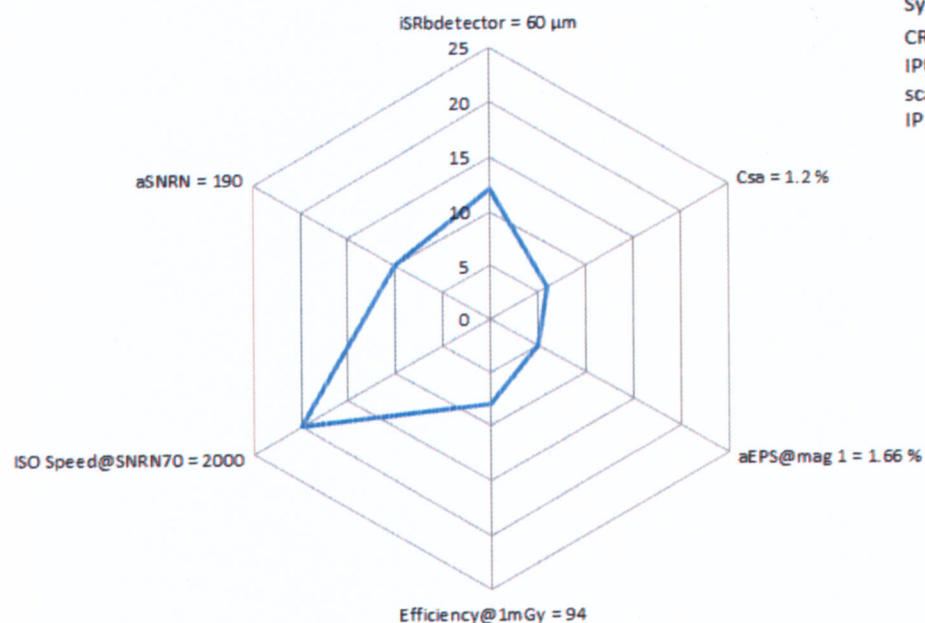

System parameters:

CR^xFlex scanner type 5176/200 S/N 2010

IPU plates LOT B3E3NU

scan resolution 50 µm

IP sensitivity 1000

Annex to
Certificate BAM/ZBF/003/16
of 2016-05-09

— Performance Level II